


IVA-2 Response Time Distribution

Name: Case, Sample

Test Date: 11/3/2014 3:10 PM Age: 31 Sex: M


Auditory Response Validity Check: Valid

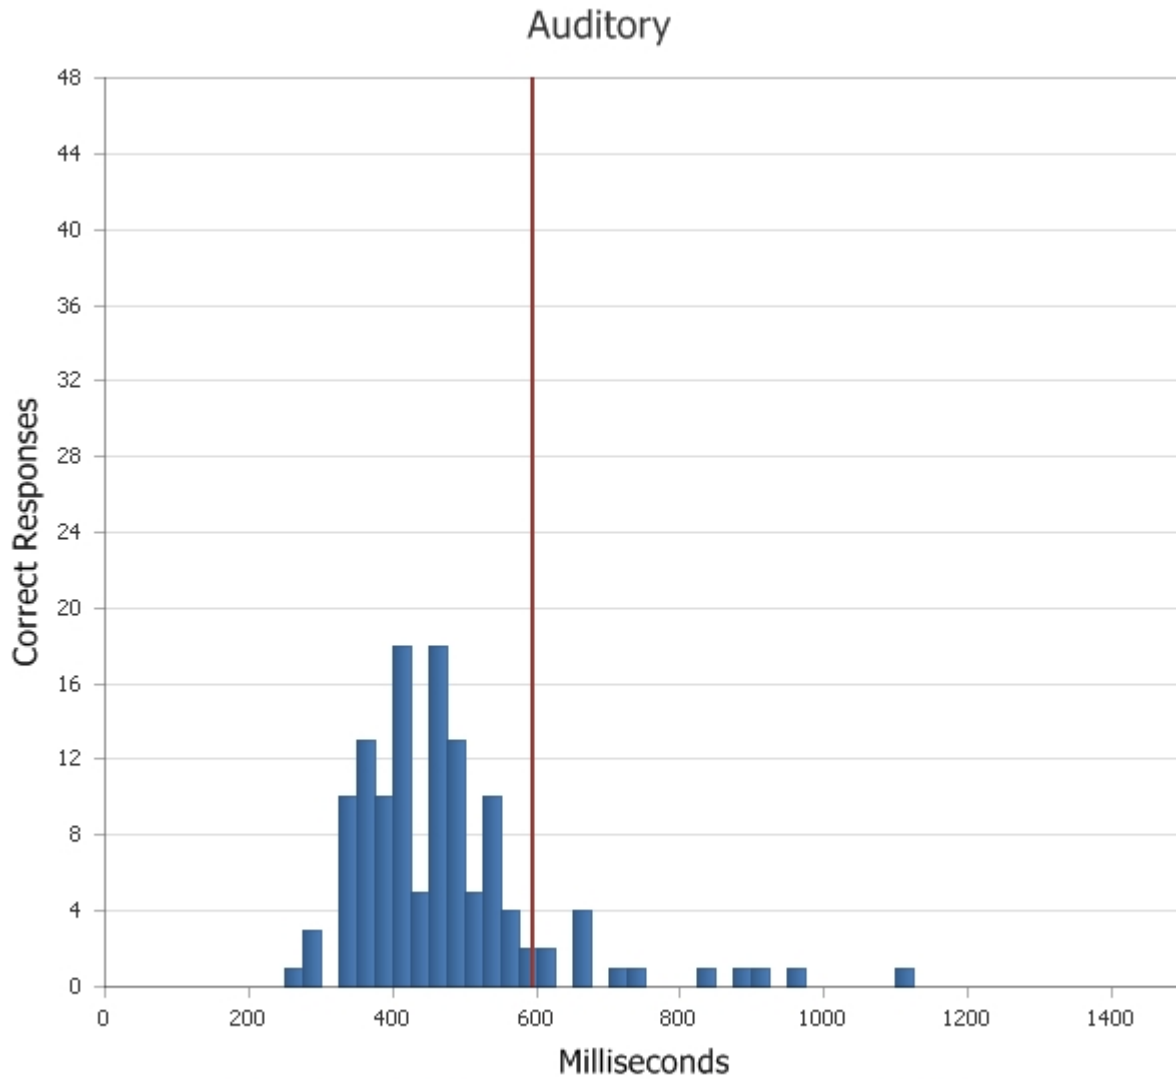

Red line indicates mean reaction time from normative database.

Accurate Responses: 125/125 (A single click to a target greater than 125 ms)
1st Quartile: 390 ms
Mean: 470 ms
3rd Quartile: 515 ms
Standard Deviation: 132 ms

Visual Response Validity Check: Valid

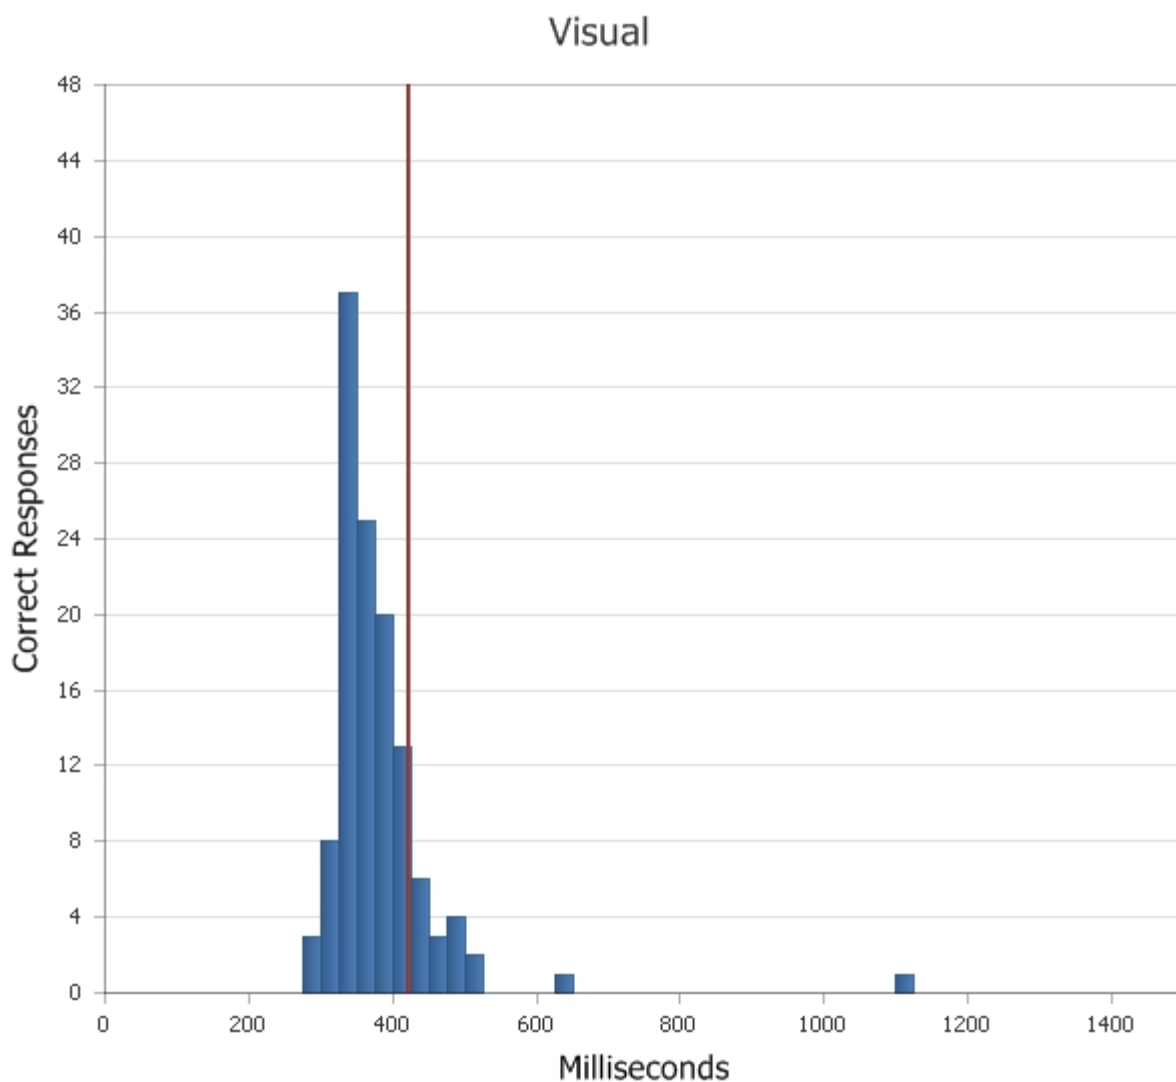

Red line indicates mean reaction time from normative database.

Accurate Responses: 123/125 (A single click to a target greater than 125 ms)
1st Quartile: 343 ms
Mean: 379 ms
3rd Quartile: 390 ms
Standard Deviation: 86 ms